

Pen peptide certificate of analysis (CoA)

Product:	AC-KPV-NH2		
Source:	Hybrid synthesis (recombinant using peptide secretion system and chemical synthesis)		
Intended use:	For stability, viability and activity testing only.		
Order number:		Lot:	25AUG21KPV
Production:	08/2025	Expiry:	08/2027
Formulation:	0.2 µm-filtered solution in 20mM glycine, 200mM Mannitol, 20mM NaH ₂ PO ₄ , pH 6.5; m-cresol 1 mg/ml, glycerol 2 mg/ml (when liquid)		
Protein/peptide concentration per 3 ml cartridge:	15 mg		

Release Testing:	Specification	Lot Result
Purity:	≥ 97%	> 98%
Identity:	Complies	Complies
Sterility:	Sterile	Complies
Endotoxin level:	< 10 EU/mg	< 0.20 EU/mg
Host-cell DNA	≤ 200 ng/mg	Complies (1.1 ng/mg)

Activity was determined using a Nb2-11 cell proliferation assay.

Purity was determined by SDS PAGE and coomassie stain (under reducing and non-reducing conditions).

Identity was confirmed by *end-of-production* DNA sequencing and N-terminal protein sequencing.

Sterility test of vialed product was performed according to Eur.Pharm. (Inoculation method).

Endotoxin was determined using the gel clot assay according to Eur.Pharm.

Host-cell DNA was determined using fluorimetric assay.

Handling Instructions:

General usage: Open cap, clean the rubber stopper with disinfectant napkin or other cleaning disinfection method / material. Puncture rubber stopper with sterile needle by screwing needle on. Remove the plastic protective cover. Set the index to physician prescribed position, remove the pink plastic cover and let out the air from the cartridge by several button presses into the air. Put on the plastic protective cover back.

Using liquid product: Liquid products are ready to use according to physician recommendations.


Storage and stability: Store material at +2 - +8°C. **Do not freeze!**

Quality Statement:

This product is manufactured, tested and realized in compliance with the relevant GMP-guidelines. No animal- or human-derived materials were used during manufacturing. USP chapter <1043> “ancillary materials for cell, gene, and tissue-engineered product” has been considered in the design of this product.

Sample Information


Product Name : KPV
Lot. No : 202508
Sequence : KPV
Column : Agilent 5 HC-C18(2) 250*4.6mm
Buffer : A: 0.1% TFA in Acetonitrile B: 0.1% TFA in H₂O
Gradient : 5-30% in 25 min
Flow rate : 1.0ml/min
Wavelength : 220nm
Dissolution method : 100% H₂O
Column temperature : 35°C

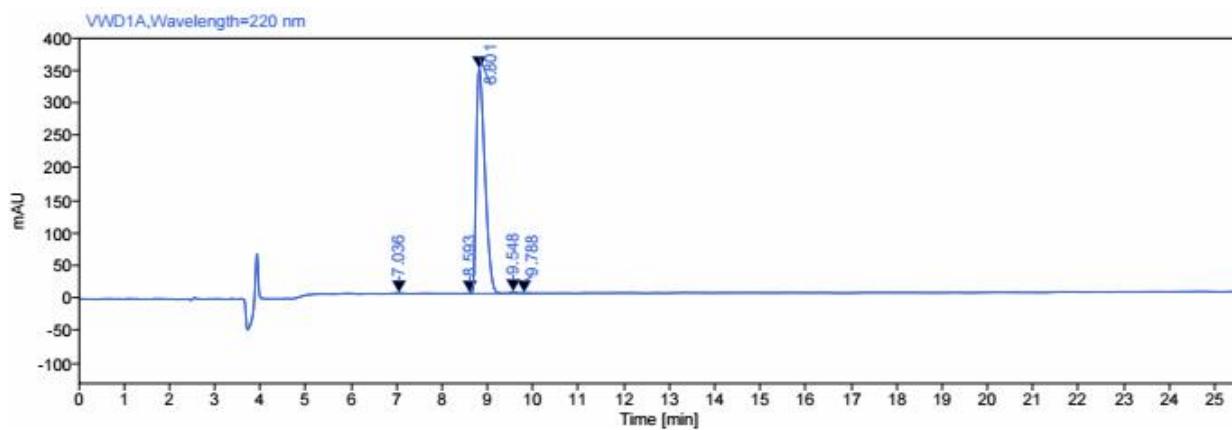

Signal: VWD1A, Wavelength=220 nm

RT [min]	Type	Width [min]	Area	Height	Area%	Name
7.036	MM m	0.21	3.69	0.68	0.08	
8.593	BM m	0.18	1.63	0.41	0.04	
8.801	MM m	0.77	4595.50	344.99	99.39	
9.548	MM m	0.33	18.23	2.25	0.39	
9.788	MM m	0.27	4.52	0.46	0.10	
		Sum	4623.58			

MS Spectrum

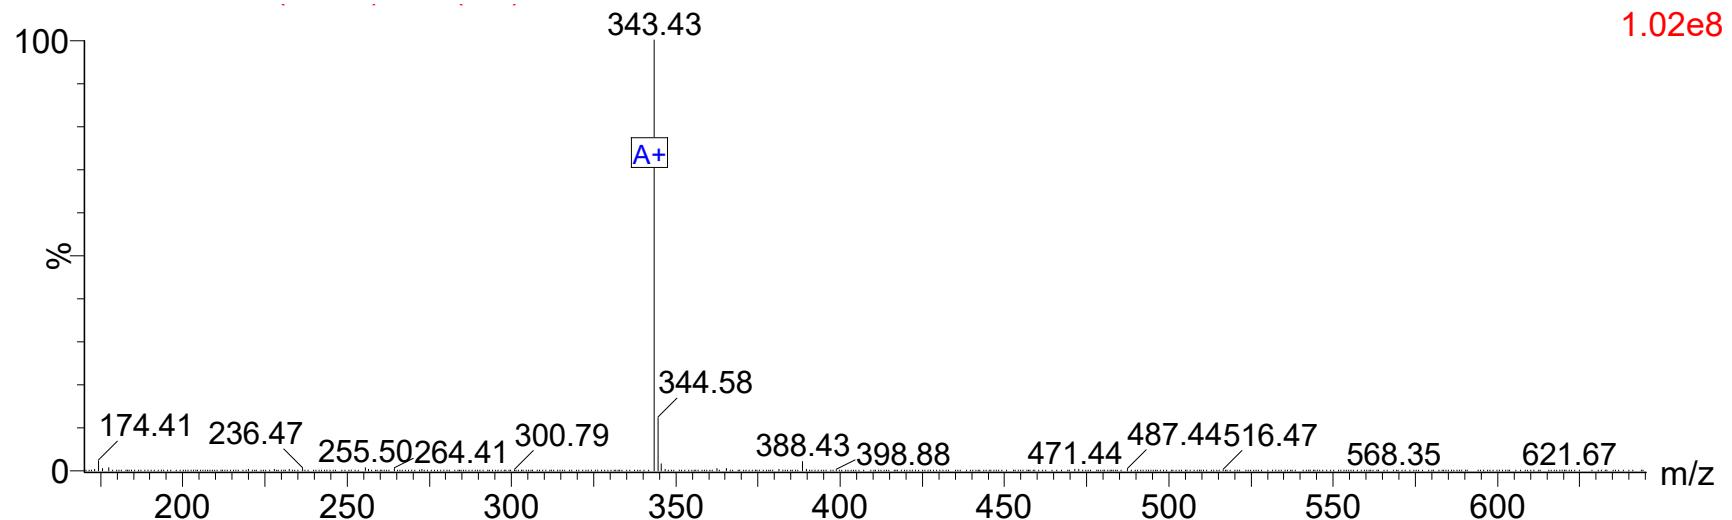

Dissolution : 0.1%HCOOH+ACN

Date : 2025/08/21

Injection 9:44:24 :2.5ul

Block Temp : 150

Interface : ESI

Nebulizing Gas Flow : 500L/hr

CDL Temp : 400C

CDL Volt : +5v

Prerod Bias

Detector

T.Flow : 0.35ml/min

B.conc : 50%H2O/50%MEOH

Product Name : KPV

Sequence : KPV

Lot.No : 202508

Theoretical : 342.43

Observed : 342.43